

JULY 2019

User Manual

CPR+
P R O M P T

Powered by **heartisense**[®]



ENGLISH

www.NascoHealthcare.com

Contents

1. Product Introduction

1.1. What is the CPR add-on kit?	3
--	---

2. Components of the product

2.1. Hardware	4
2.2. Software	5

3. Installing the hardware

3.1. Installing the Add-on kit	6
3.2. Installing the lung bag	7

4. Installing the software

4.1. Installing the apps	8
--------------------------------	---

5. Before using

5.1. Checking the power of the Add-on kit	9
5.2. Checking the Add-on kit's ID	9

6. Main features of the application

6.1. Tab menu	10
6.2. Learning using the Student app	11
6.3. Training using the Instructor app	13

7. Feedback & Graph UI

7.1. Compression & Breath Feedback UI	17
7.2. Graph UI (for Instructor app only)	17

8. More Features

8.1. Reviewing saved data	18
8.2. Exporting the result/certificate as a PDF file	19
8.3. Renaming the manikin	20
8.4. Renaming the student name (for Instructor app only)	21
8.5. Checking the connected kit information	22
8.6. Changing the settings	23

9. Maintenance

9.1. Checking the remaining battery level of the Add-on kit	24
9.2. After using the Add-on kit (Power on/off)	24
9.3. Replacing the breath module when it has a problem	25
9.4. Attaching the sensor holder when replacing the lung bag	25

10. Troubleshooting

10.2. Frequently Asked Questions	26
10.2. Troubleshooting	27

11. Warranty

12. Contact

1. Product Introduction


1.1. What is the CPR add-on kit?

As a sensor kit attached to the dummy manikin, the CPR add-on kit provides feedback regarding the CPR action in real-time, allowing users to have a complete training experience. CPR feedback can be received in real time by connecting the Add-on kit installed on the manikin to the mobile application. The application provides feedback for the compression (depth, recoil, rate), breath (volume) and hands-off time in real-time, and the feedback and evaluation standard meets the latest guideline of the American Heart Association (AHA). CPR add-on kit apps for Add-on kit consist of Student and Instructor apps.


CPR add-on kit 4points

 <p>Compliance with AHA Guideline</p>	 <p>Real-time feedback</p>	 <p>Quantitative measurement</p>	 <p>Intuitive system</p>
--	---	--	---

CPR add-on kit Student

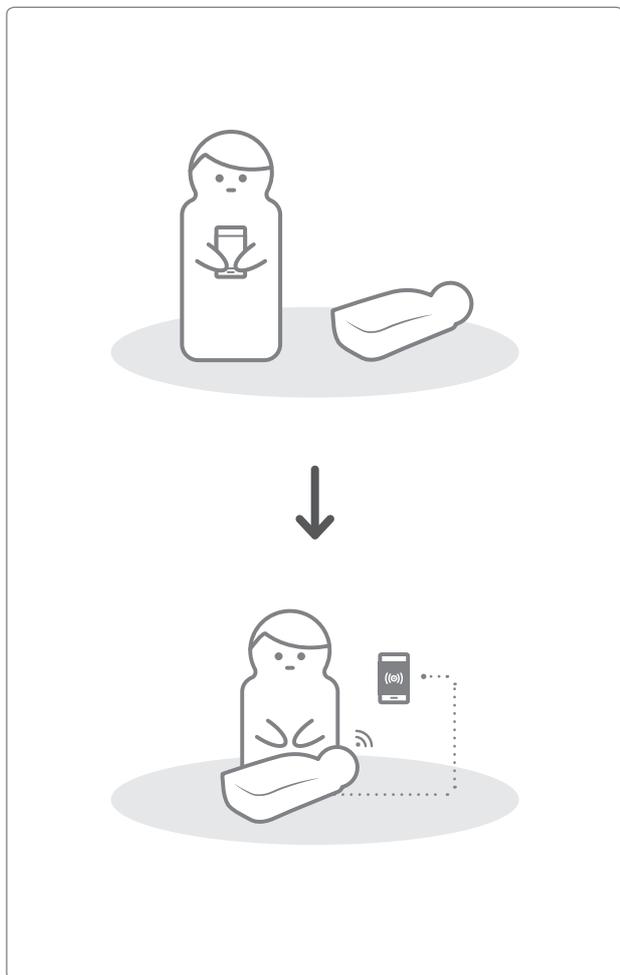

CPR add-on kit Instructor

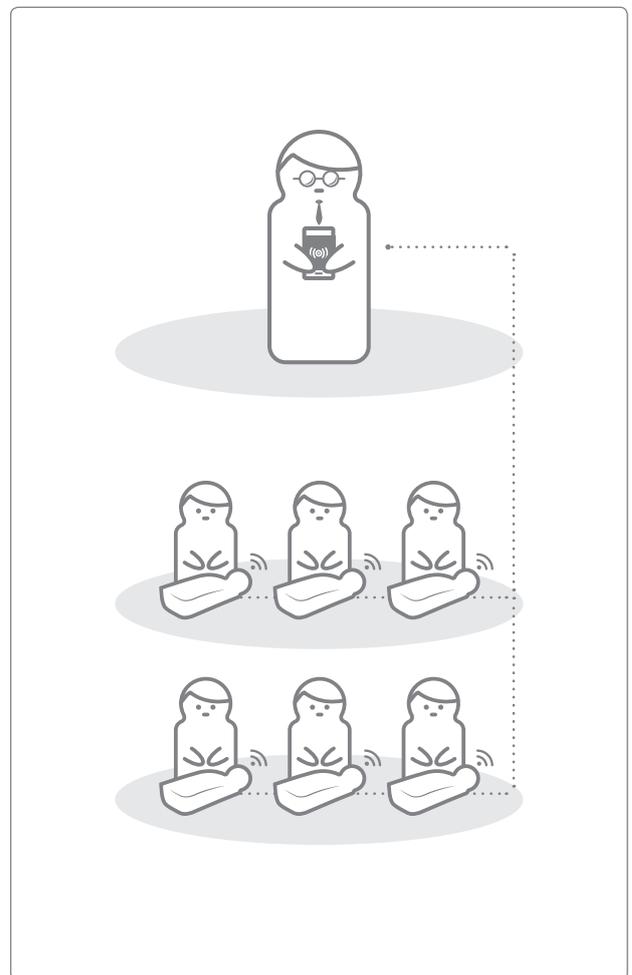


2. Components of the product

2.1. Hardware


Add-on kit

The Add-on kit equipped with the sensor in the correct form for each manikin sends compression and breath data to the mobile device in real time.

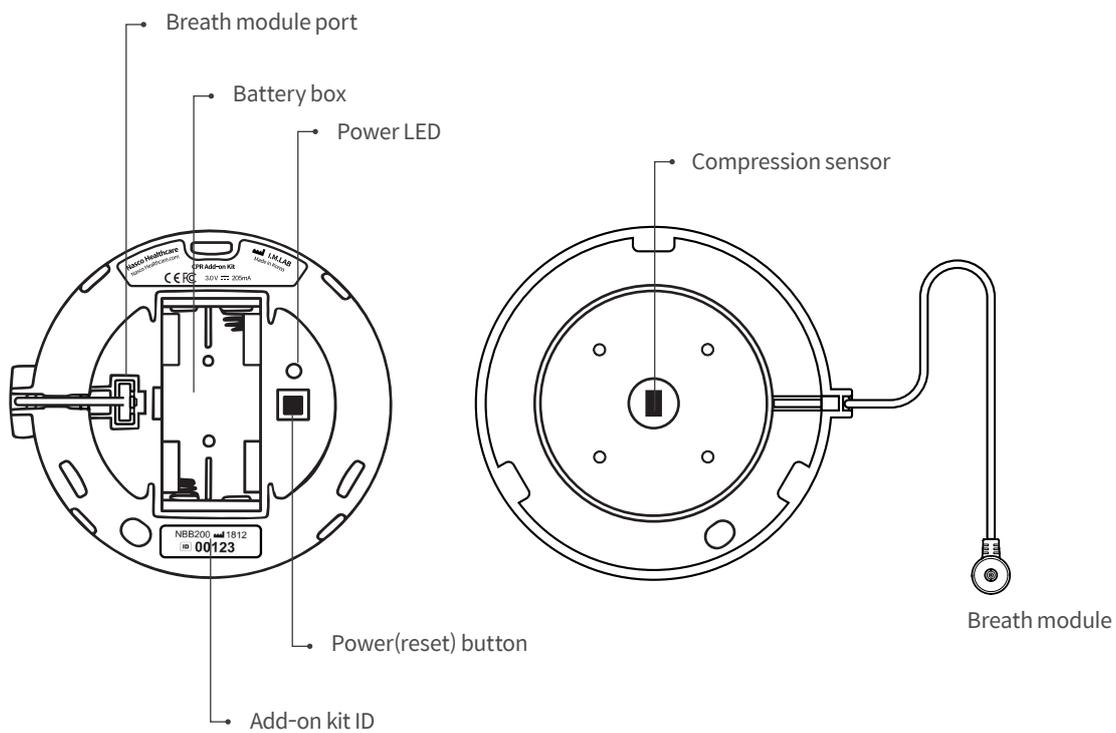

Lung bag

The lung bag is connected to the breath module and used for measuring the volume and timing of breath.

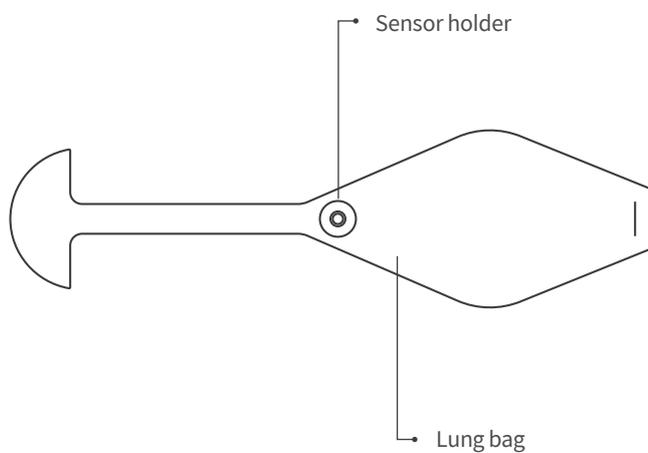

2.2. Software

CPR add-on kit Student

The Student app is a learning application and this software analyzes CPR carried out by a student in real time and gives feedback.



- Measures the CPR performance and gives feedback
- Saves and converts measured data into a score
- Reviews and exports the saved score

CPR add-on kit Instructor

The Instructor app is a training application that enables the monitoring of CPR carried out by a student in real time and this software helps with evaluation, recording and management.



- Supports connection with up to 6 manikins and feedback
- Measures the CPR performance and gives feedback
- Saves and converts measured data into a score
- Reviews and exports the saved score

Supported device and version



Android Devices

Android 7.0 (Marshmallow) or above.
BLE 4.2 or above.




iOS Devices


OS 11.0 or above.
BLE 4.2 or above.

3. Installing the hardware


3.1. Installing the Add-on kit

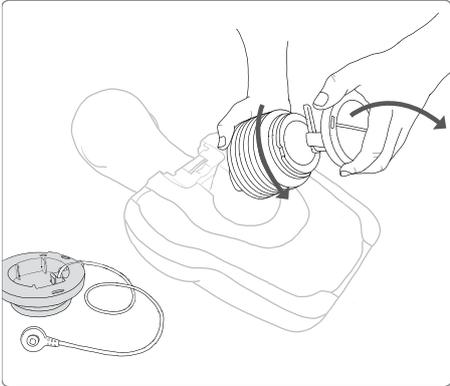

- 1) Turn over the manikin and take out the piston.
Turn the bottom part of the piston counterclockwise to separate it from the piston itself.

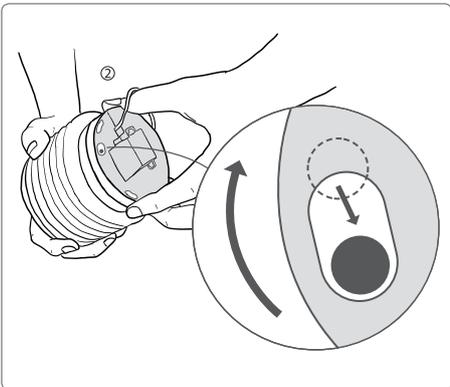


- 2) Line up Add-on kit into the piston with edges aligned, and press down while turning it to assemble Add-on kit into the piston. It is easier if you refer to the hole right next to the kit ID label (as shown on the picture on the left).

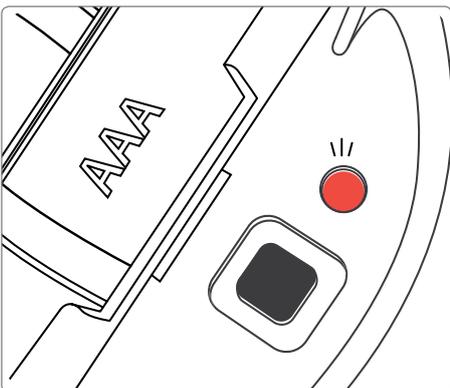


- 3) Place the breath module in the direction of the manikin head while considering the connection with the lung bag.


3.2. Installing the lung bag

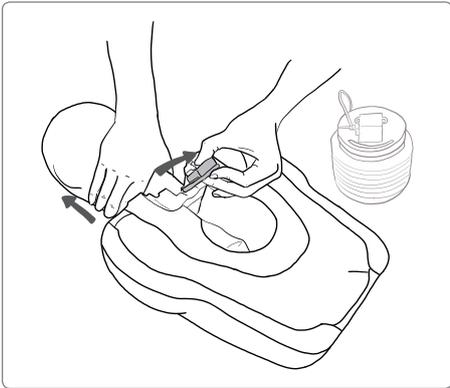

- 1) Remove the locking clip at the back of the manikin to separate the head from the body.

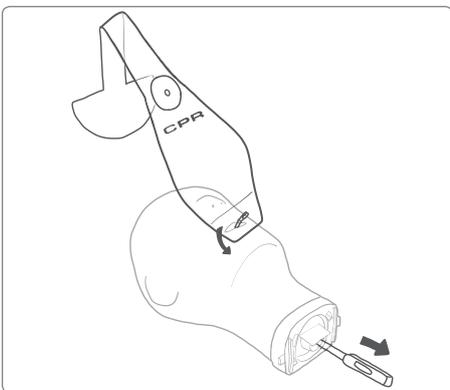

- 2) Use the hook to pull the lung bag through the manikin head towards the neck.

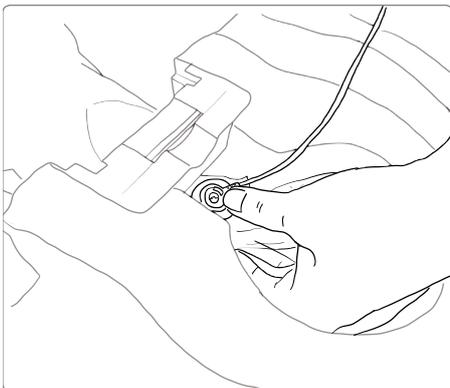


- 3) Assembly the head back to the body and attach breath module to the sensor holder on the lung bag.




- 4) Assembly the piston back to the manikin body while the battery compartment facing up.

4. Installing the software

4.1. Installing the apps

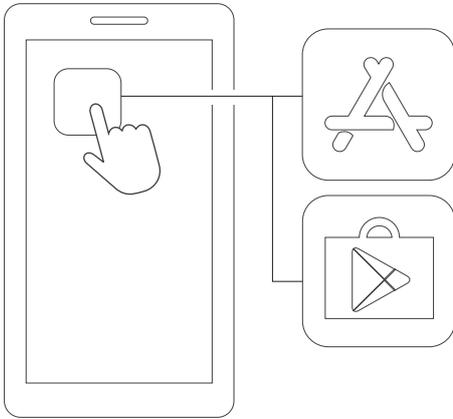

1) Connect to the App Store (iOS) or Google Play Store (Android).



2) Search for CPR add-on kit.



CPR add-on kit
Student

3) Download the Student app and the Instructor app.




CPR add-on kit
Instructor




5. Before using

5.1. Checking the power of the Add-on kit

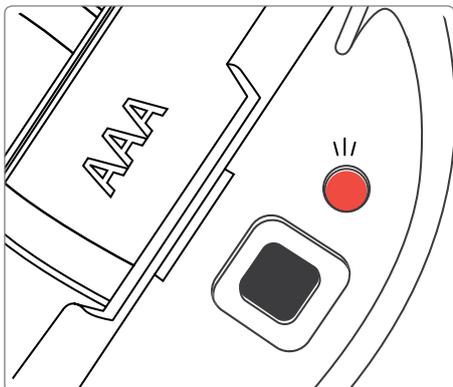

- 1) If there is no sensor input for 10 minutes while the power is ON, the Add-on kit will be turned off automatically to save power.
- 2) Check its ON status through the LED lamp at the bottom of the kit.

5.2. Checking the Add-on kit's ID

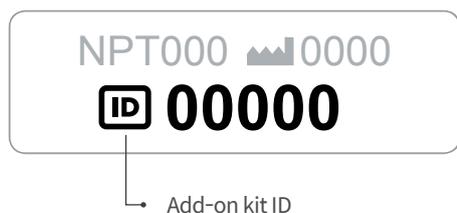

Check the ID from the label attached to the back of the Add-on kit. ID is used for connecting the Add-on kit and the application via Bluetooth.

6. Main features of the application

6.1. Tab menu

CPR add-on kit Student



The CPR add-on kit Student consists of the following tabs.



Training

You can monitor CPR performance in real time.



Results

You can manage saved training records.



Settings

You can adjust the settings applied to the training including the guideline and score calculation settings.

CPR add-on kit Instructor



The CPR add-on kit Instructor consists of the following tabs.



Training

You can select the measurement method and monitor CPR performance in real time.



Link

The connected manikin information is displayed, allowing you to check the status before carrying out training.



Data


You can manage saved training, evaluation records and student list.



Settings


You can adjust the settings applied to the training including the guideline and score calculation settings.

6.2. Learning using the Student app

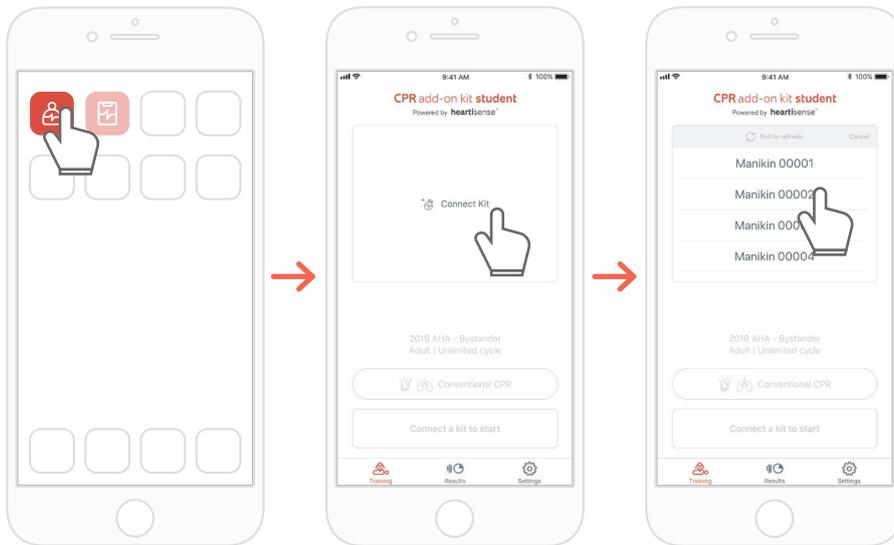

- 1) Run the CPR add-on kit Student and then select Connect Kit on the main screen.
- 2) Select the desired manikin ID from the list to begin the Bluetooth connection.

*The ID of the kit is provided at the back of the product, and refer to '5.2 Check Add-on kit ID' for detailed information.

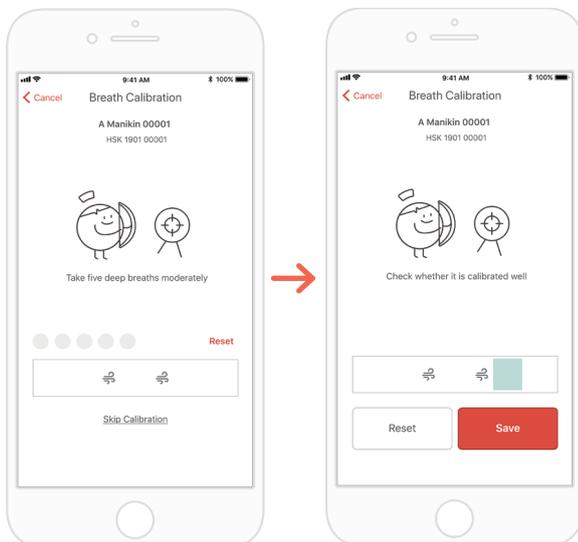

- 3) When the kit is connected to the app for the first time, the breath module should be calibrated. The calibration screen will pop up automatically.

*Deliver a proper volume of breath 5 times as instructed on the screen and press the Save button.



4) When the Bluetooth connection is made successfully, the manikin information will be displayed on the screen. Select the evaluation item(s), measuring compression only or both compression and breath.

* You can calibrate the breath sensor by selecting the target-shaped icon.



If the breath sensor is calibrated



If the breath sensor is not calibrated



* You can set the metric of measurement




Evaluation is carried out based on the hands-only CPR.



Evaluation is carried out based on the CPR (30:2).

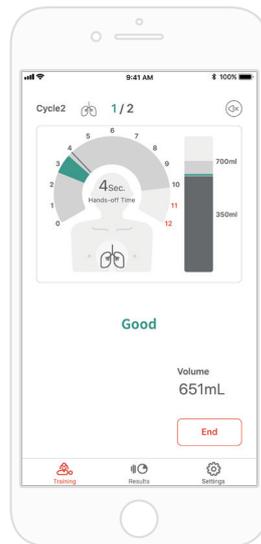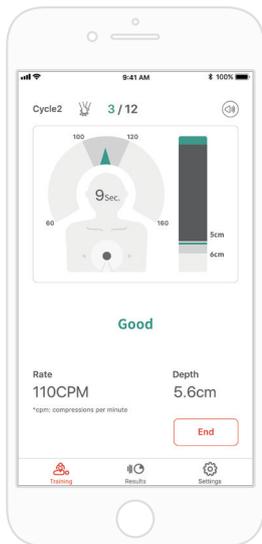

After the session →

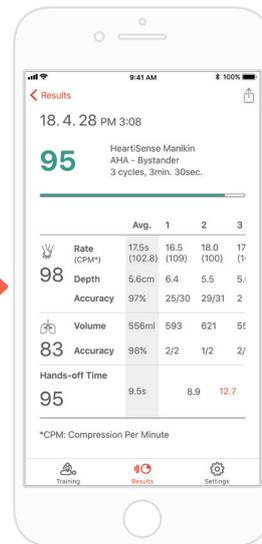


5) When a user performs CPR, the application gives feedback for the compression or breath.


*Refer to '7.1 Compression & Breath Feedback UI' for information regarding the feedback displayed on the screen.

6) When CPR is completed, the measured data will be shown in numerical figures.


6.3. Training using the Instructor app

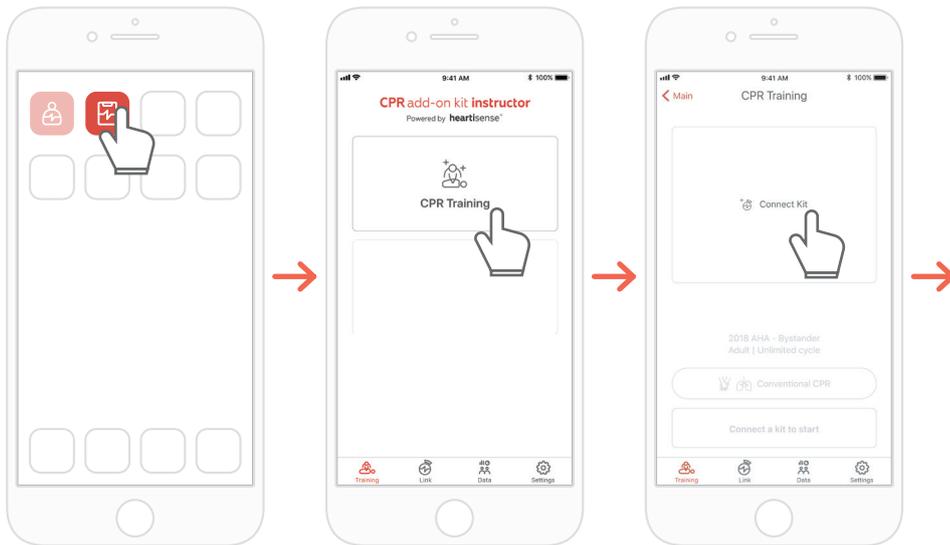


- 1) Run the CPR add-on kit Instructor and select 'CPR training' on the main screen.
- 2) When you press 'Connect Kit', available kits for connection will be showed.

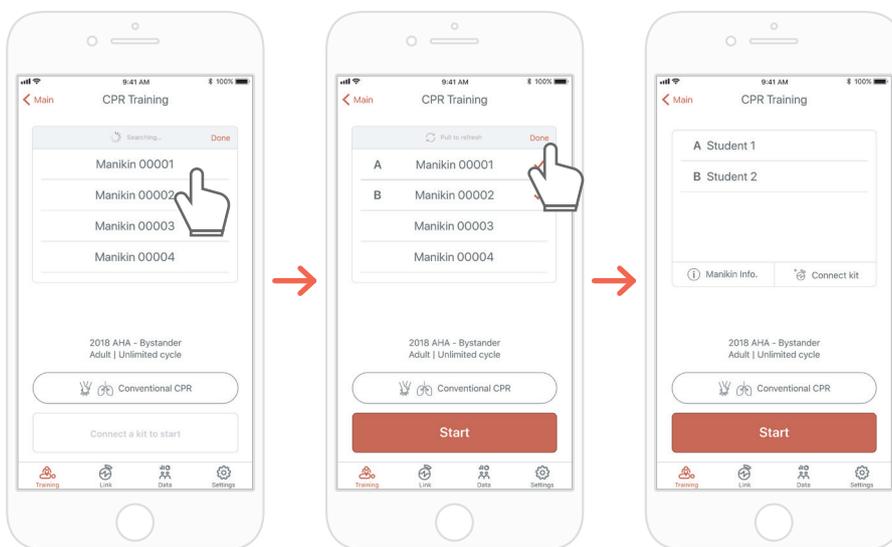

- 3) Select the manikin name you wish to connect from the list and try the Bluetooth connection.
 - 4) When the connection is made, press the 'Done' button to end searching for kits
- *The ID of the kit is provided at the back of the product, and refer to '5.2 Check Add-on kit ID' for detailed information.

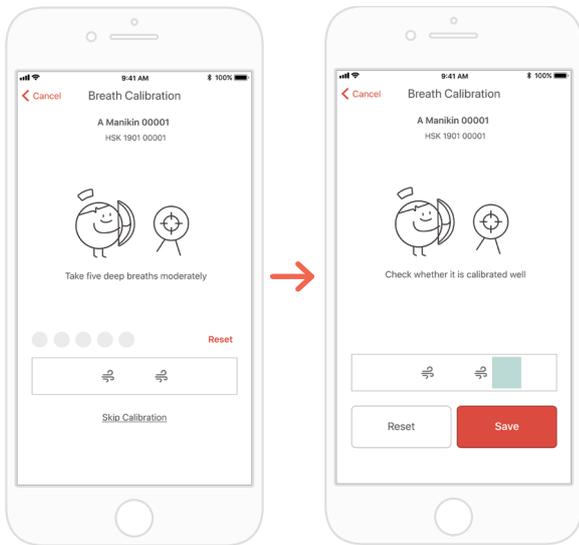

- 5) When the kit is connected to the app for the first time, the breath sensor should be calibrated. The calibration screen will pop up automatically.
 *Deliver a proper volume of breath 5 times as instructed on the screen and press the Save button.

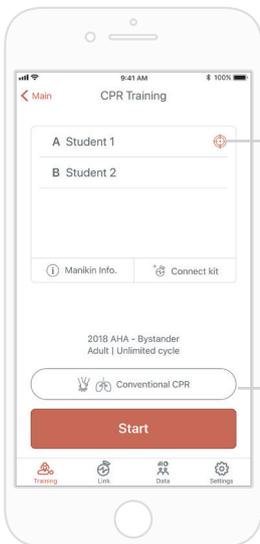


- 6) When the Bluetooth connections are made successfully, students will be shown on the screen.

* You can calibrate the breath sensor by selecting the target-shaped icon.



If the breath sensor is not calibrated


* You can set the metric of measurement



Evaluation is carried out based on the hands-only CPR.




Evaluation is carried out based on the CPR (30:2).

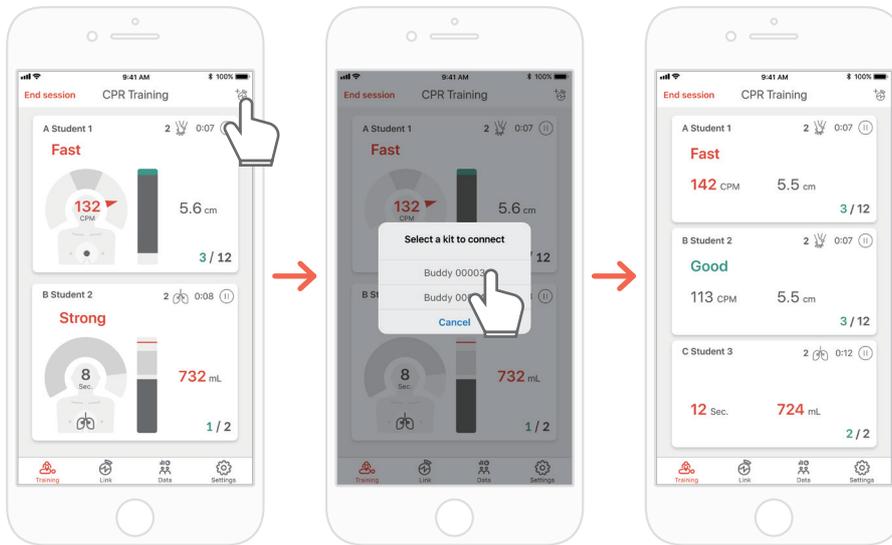

7) The CPR add-on kit Instructor app can monitor up to 6 students.


You can add a kit through the icon on the top right side while evaluating.

*Refer to '7.1 Compression & Breath Feedback UI' for information regarding the feedback displayed on the screen.

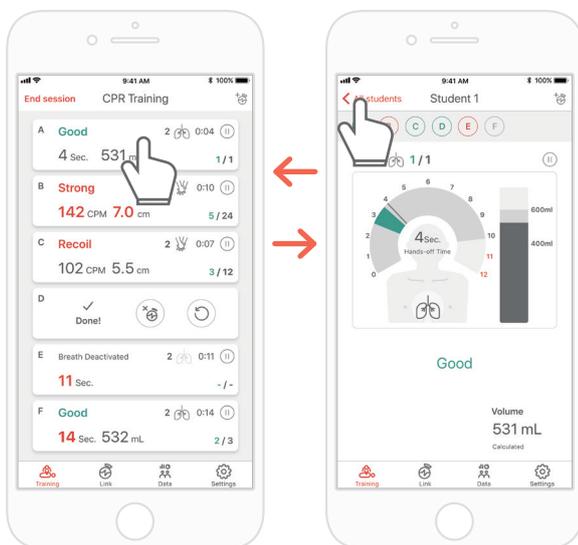

8) If there is a student marked with red text, you can select the slot and check the problem in detail.

*On the 'Detailed view' screen, you can press the back arrow button to return to the previous screen or press the alphabet button to move to a different slot..

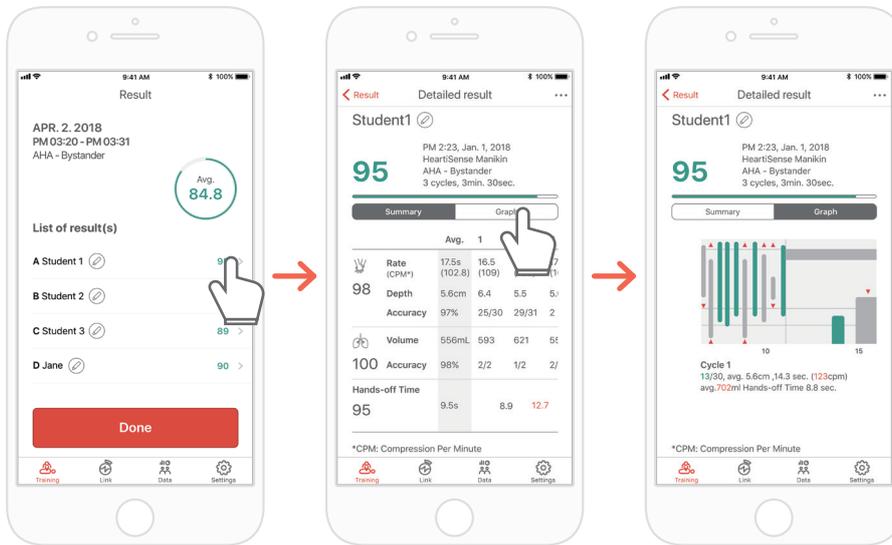


9) You can review CPR performance data in the form of a summary or graph.

*Refer to '7.2. Graph UI (Instructor app)' for information regarding graph view

To connect a number of manikins at the same time, connect them from the list in consecutive order and press the 'Done' or 'Start' button without searching for them repeatedly.




If there is a kit which is not calibrated among the kits, the calibration screen for the relevant kit will pop up immediately. You can connect manikins continuously after completing the calibration.

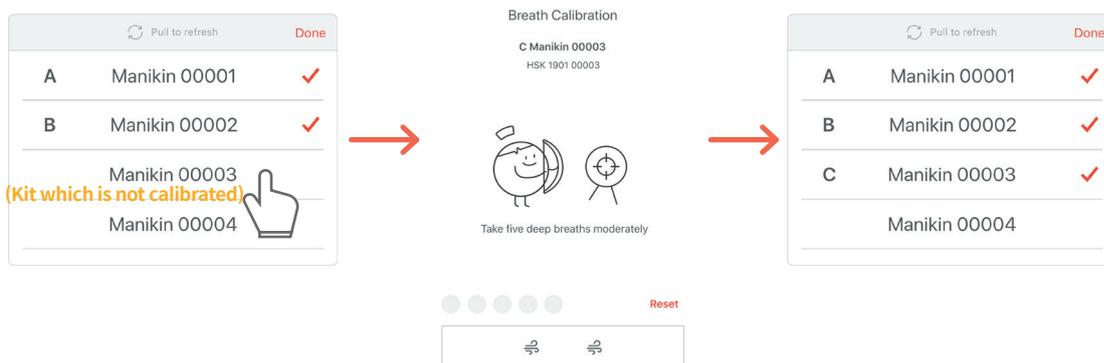


7. Feedback & Graph UI

7.1. Compression & Breath Feedback UI

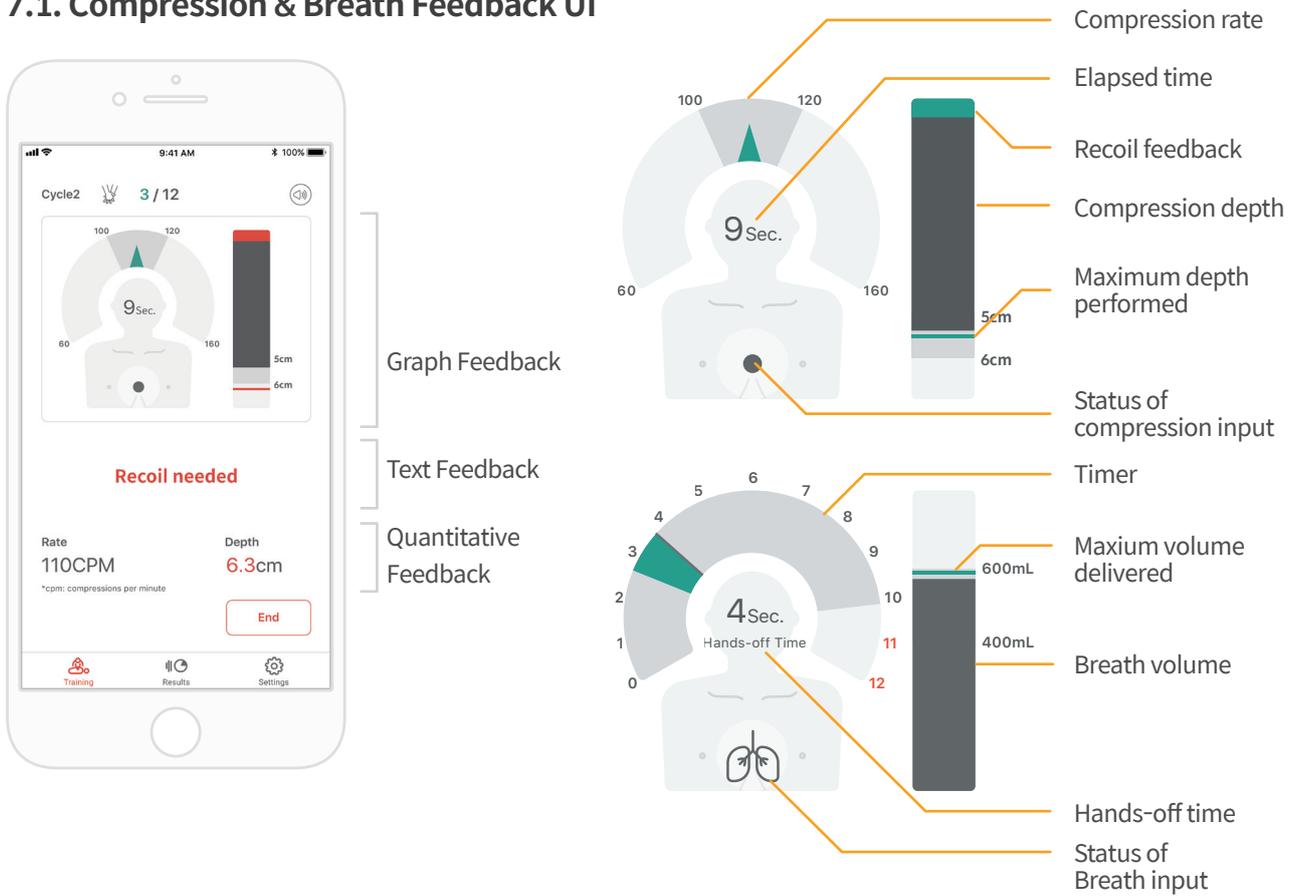


7.2. Graph UI (for Instructor app only)

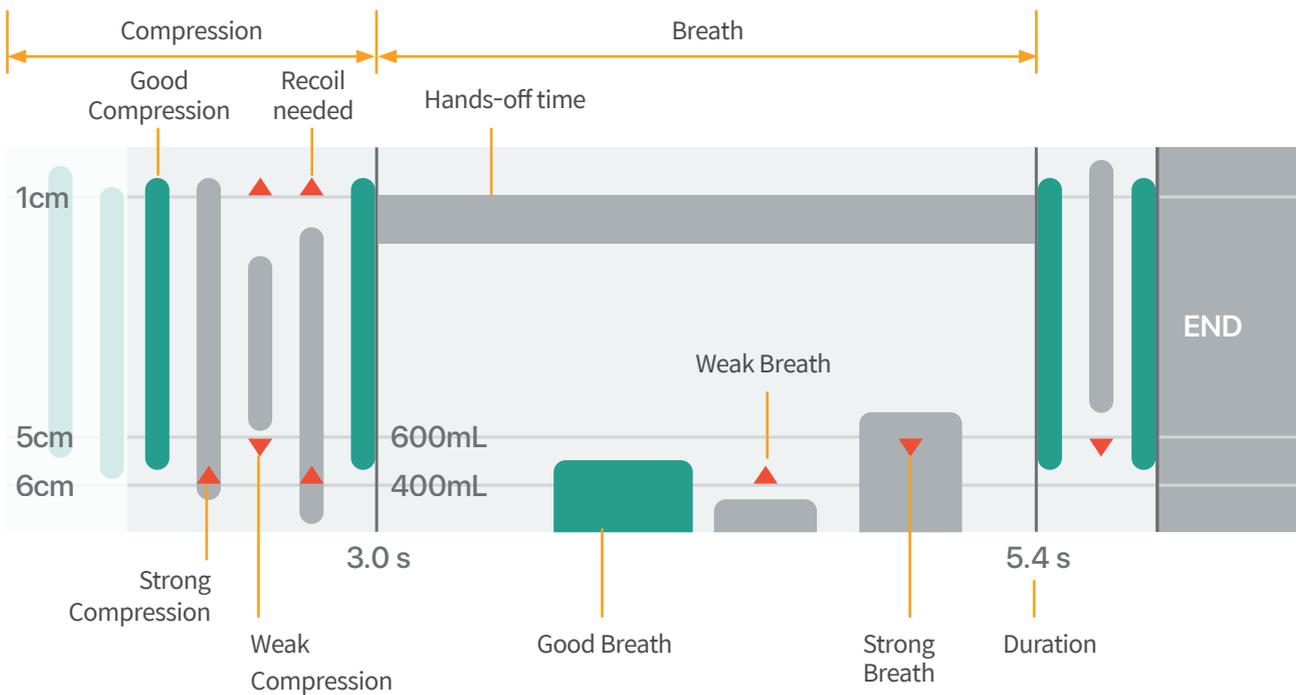


8. More Features

8.1. Reviewing saved data

CPR add-on kit Student

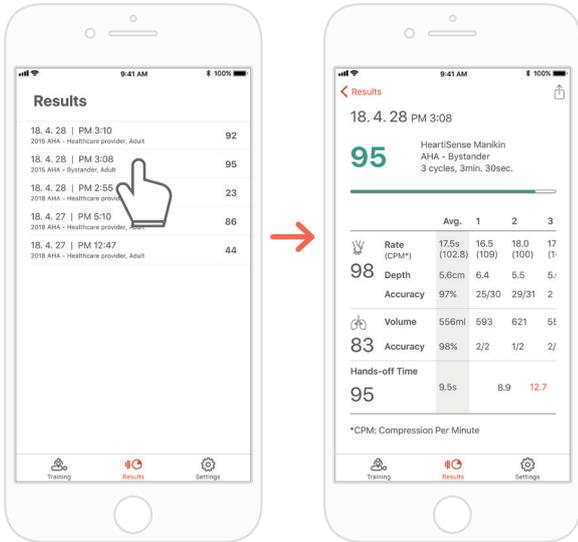

CPR add-on kit Instructor

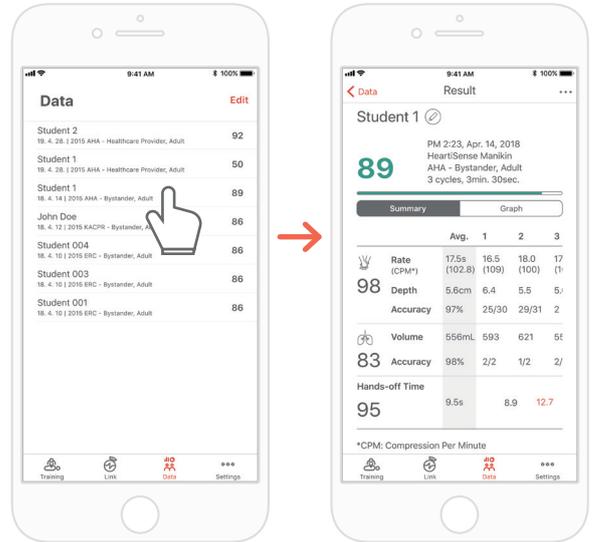


The 'Result' tab of the Student app




The 'Data' tab of the Instructor app


Deleting the result from the list (common for both the Instructor and Student apps)

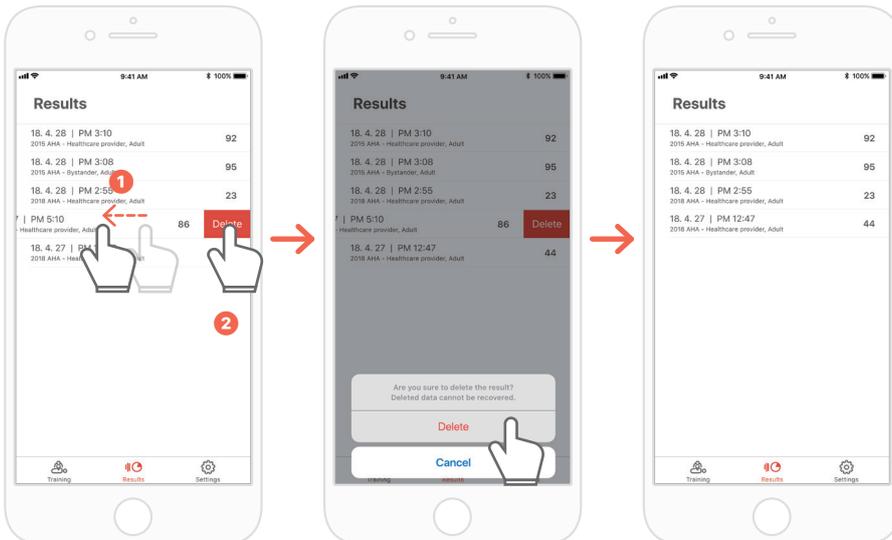

8.2. Exporting the result/certificate as a PDF file

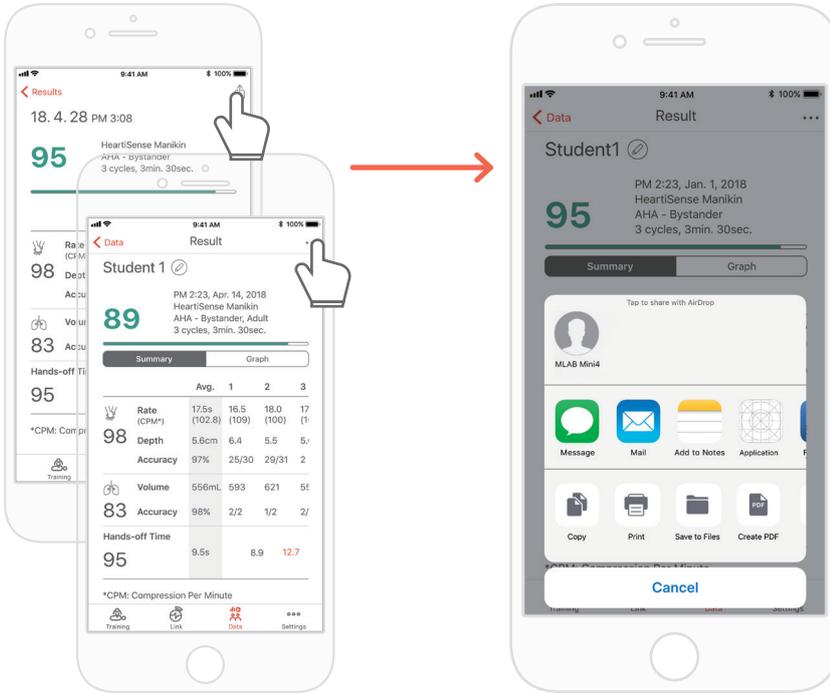


You can print the results or export PDF files to other apps by clicking the top right icon in the individual(detailed) results of the Student / Instructor app.

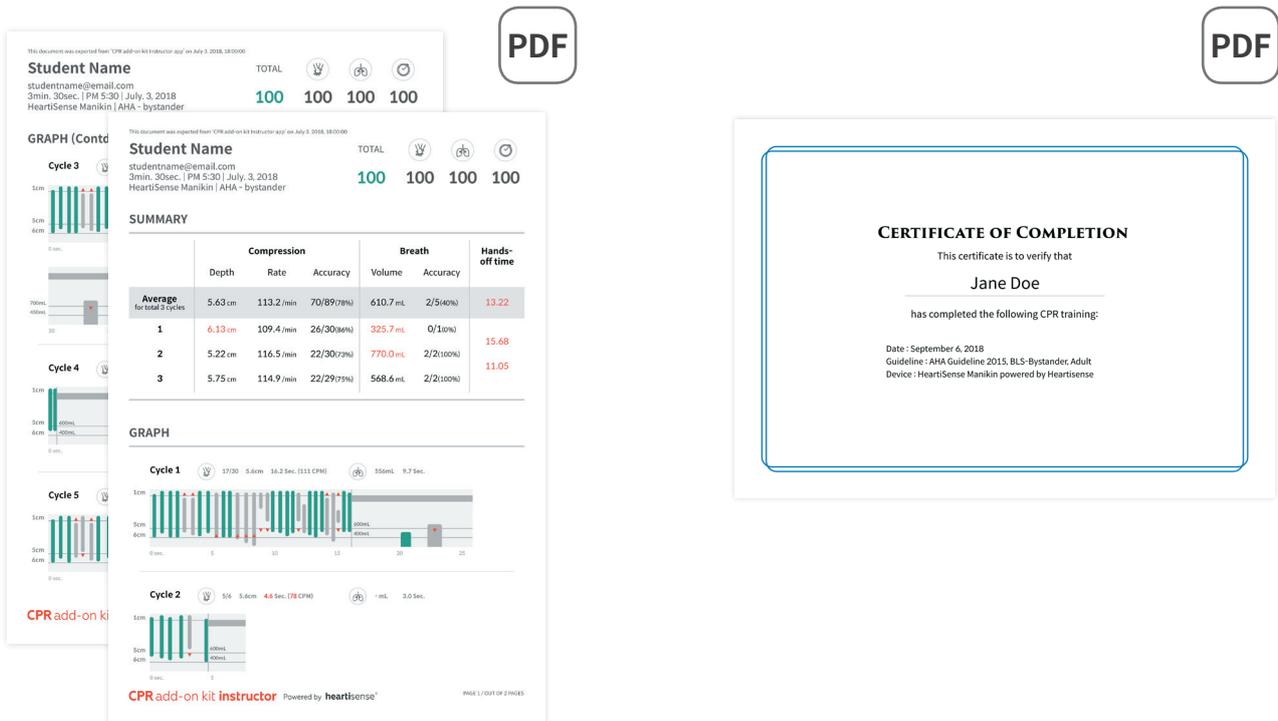

Result sheet (left) and certificate (right). Certificates can only be exported from the Instructor app.

8.3. Renaming the manikin

CPR add-on kit Student app

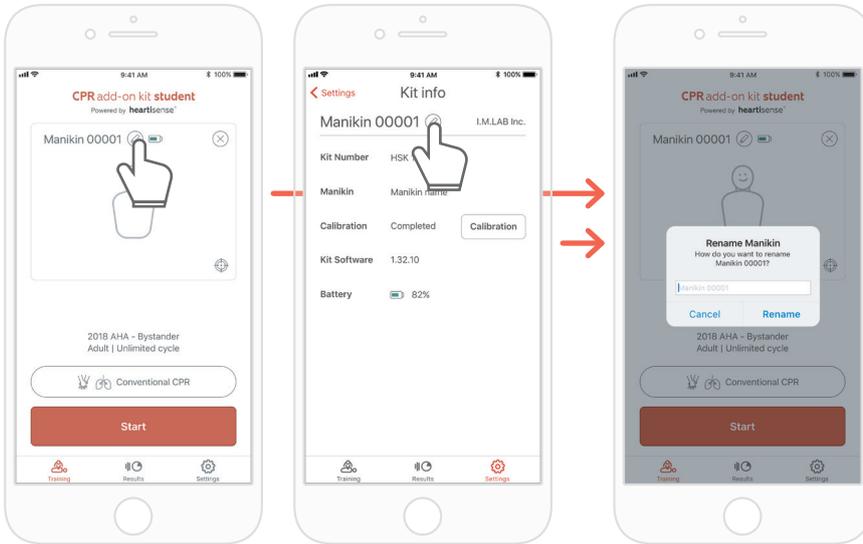


When the manikin is renamed, it will be saved in the kit so that the changed name will be displayed at the next connection.

The manikin name can be up to 15 alpha-numeric characters.

You can rename the manikin by pressing the pencil-shaped icon next to the manikin name.


CPR add-on kit Instructor app

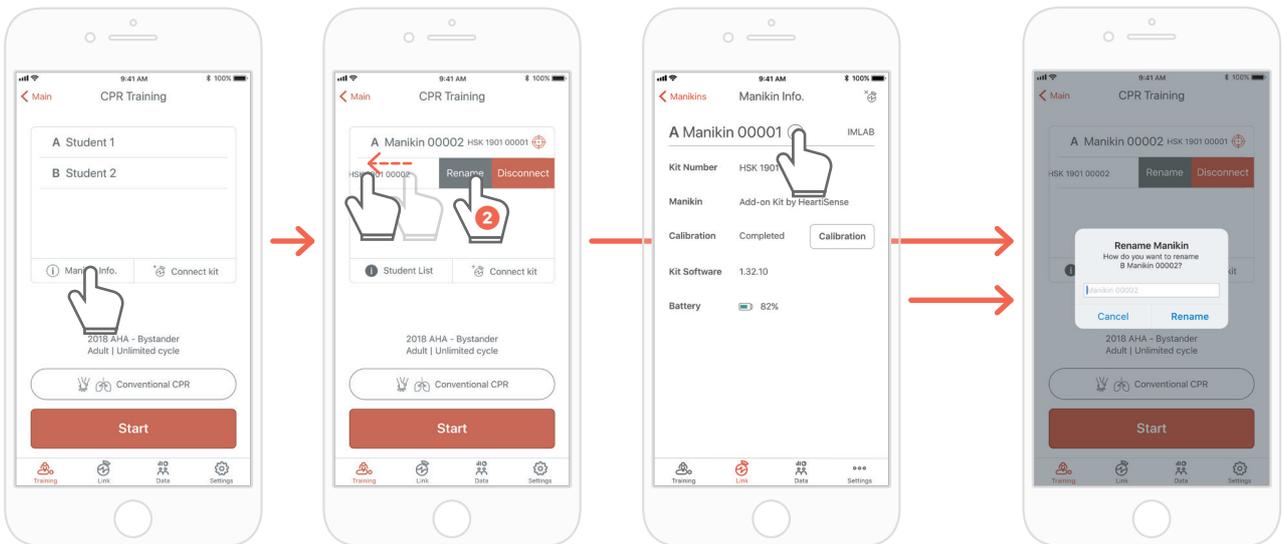

When you display the manikin list and push the slot whose name you intend to change to the left, the Rename button will be displayed. You can also rename it from the kit information on the Link tab.

8.4. Renaming the student name (for Instructor app only)


Renaming the student for each slot

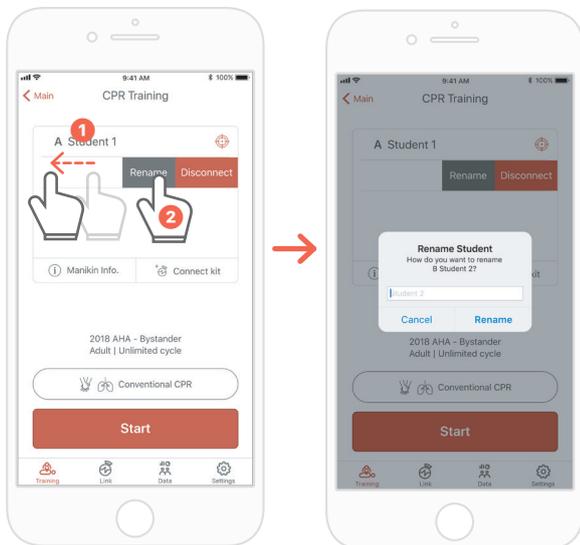

You can change the relevant student name by pushing the slot to the left.


*The changed student name is maintained while the relevant connection is maintained, and the result will be saved under the changed name..

Renaming the student for the result

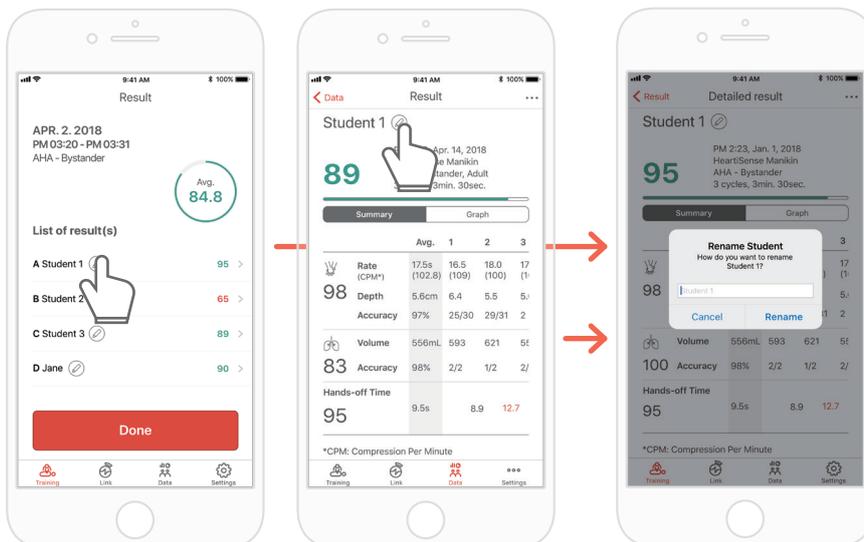


8.5. Checking the connected kit information

CPR add-on kit Student

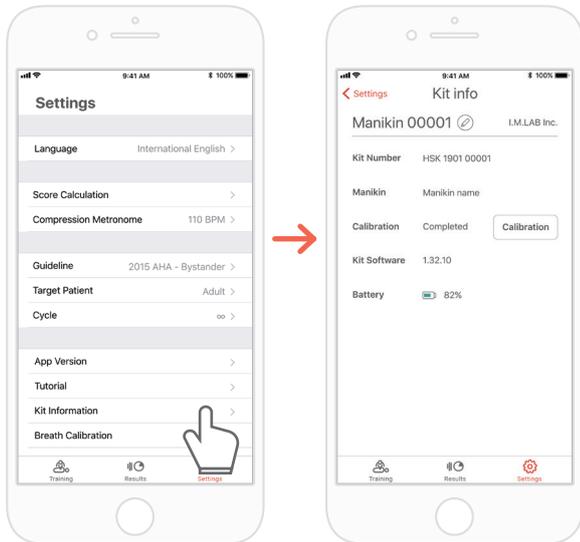


The 'Settings' tab of the Student app
→ 'Kit Information'

CPR add-on kit Instructor

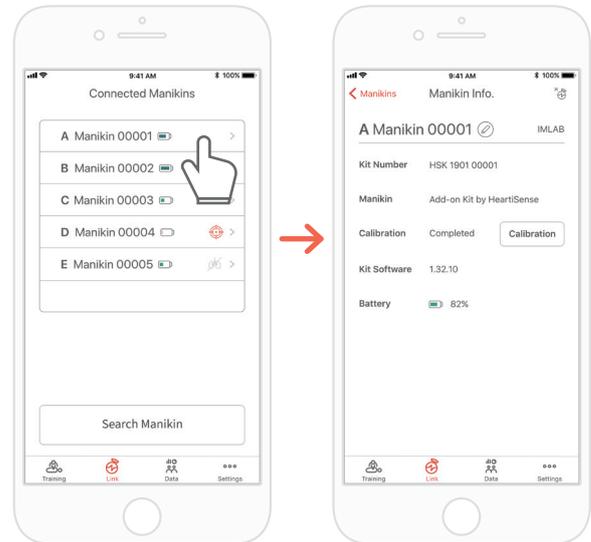


The 'Links' tab of the Instructor app
→ Select the manikin desired to
check its detailed information


Calibrating the breath sensor again from the kit information (common for the Instructor and Student apps)

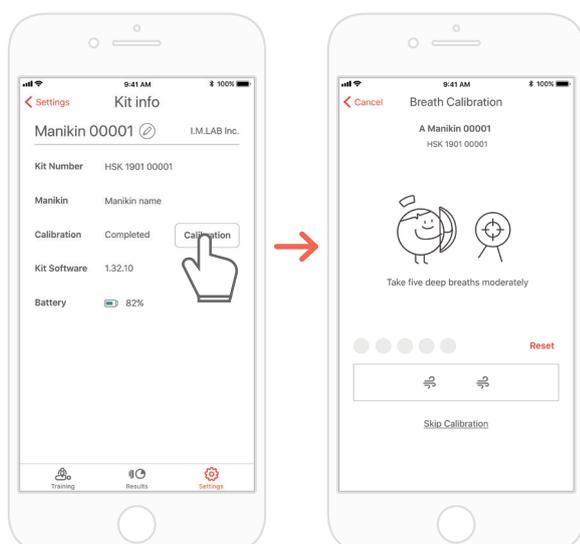

8.6. Changing the settings

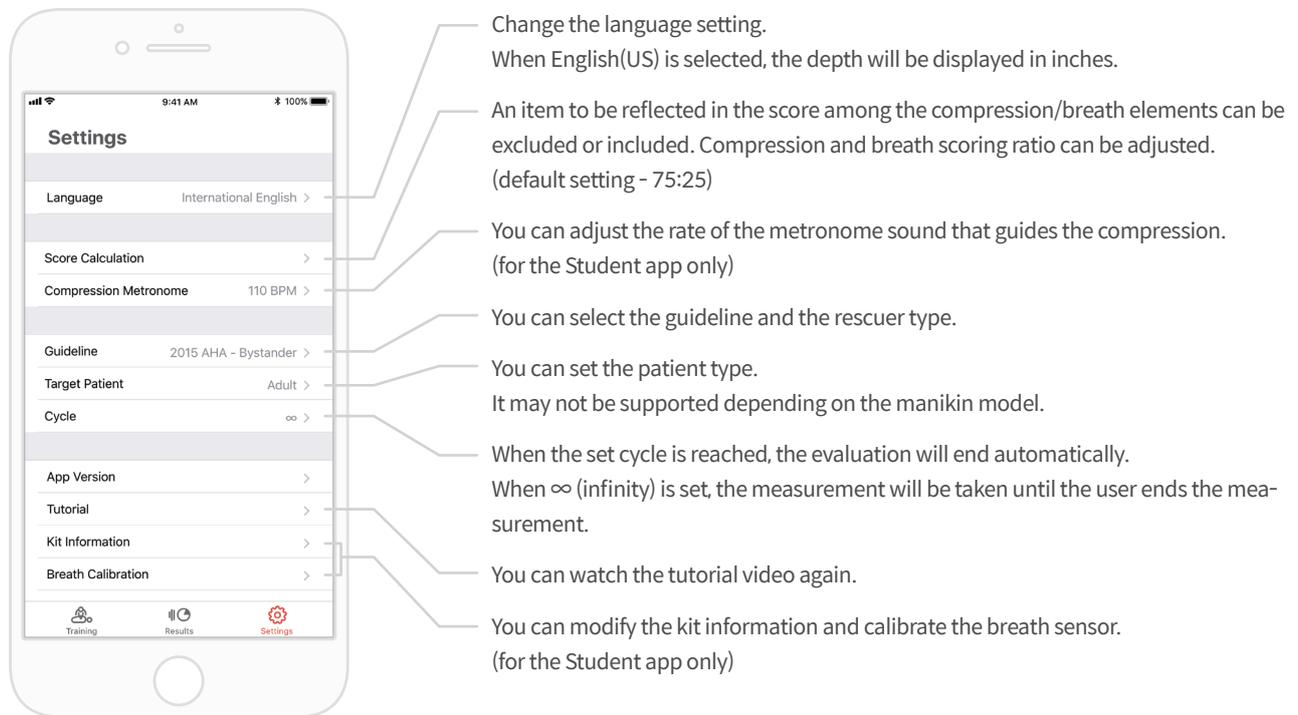


Checking the version of the current app

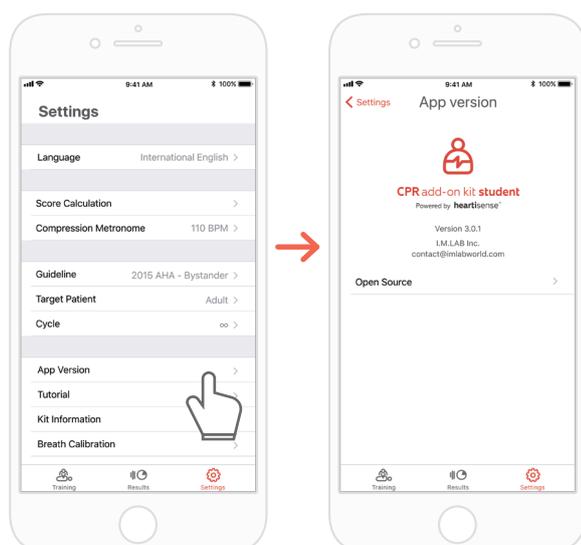

9. Maintenance

9.1. Checking the remaining battery level of the Add-on kit

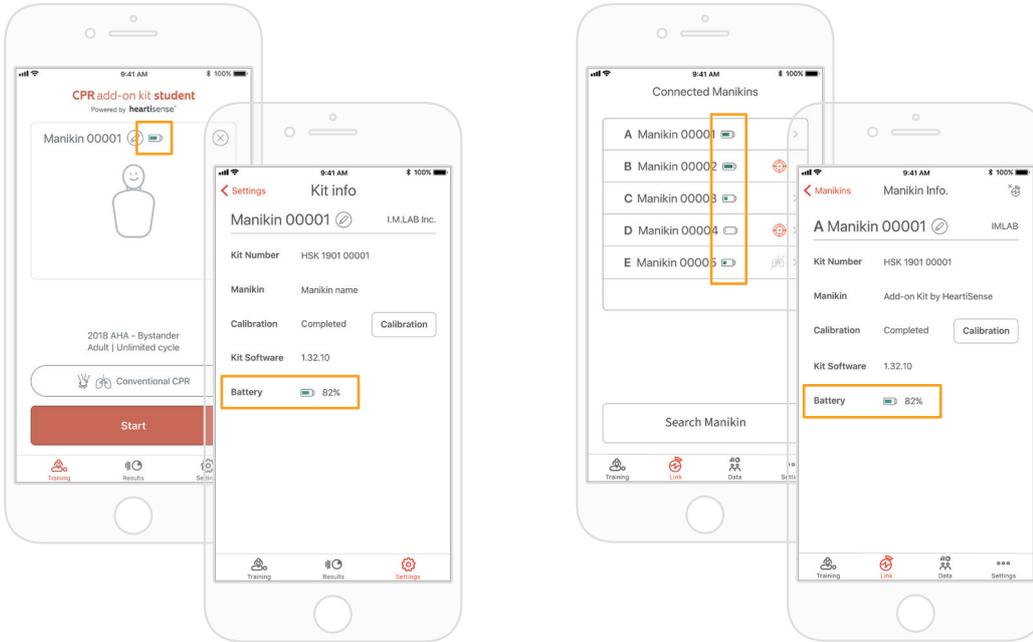


Check it from the kit information on the 'Training' main screen or 'Settings' of the Student app.



Check it from 'Link' or the Manikin Info of the Instructor app.


9.2. After using the Add-on kit (Power on/off)

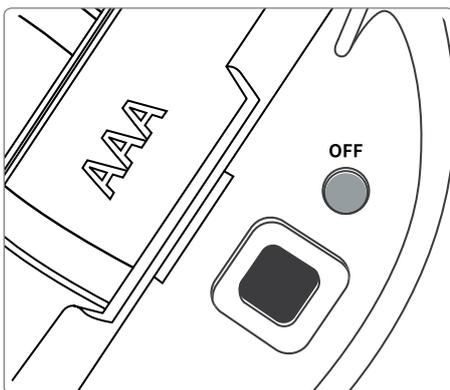

If there is no sensor input for 10 minutes while the power is ON, the kit will be turned off automatically to save power.

'When the kit is turned off, it is recommended to store the kit after separating the battery from the kit.


9.3. Replacing the breath module when it has a problem

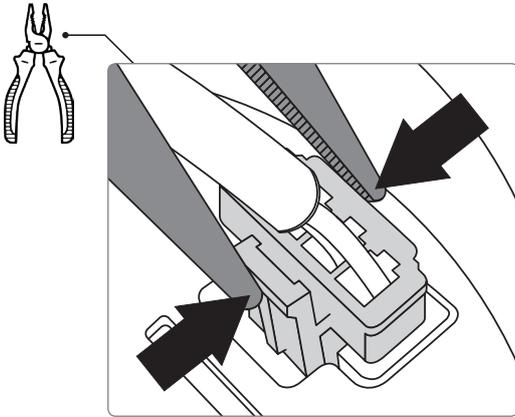

If the breath module is connected properly but the breath value is abnormal repeatedly, the breath module cannot be used any more and it should be replaced.


Separate the breath module from the kit using the tool (long-nose plier is recommended) and install a new breath module.

9.4. Attaching the sensor holder when replacing the lung bag

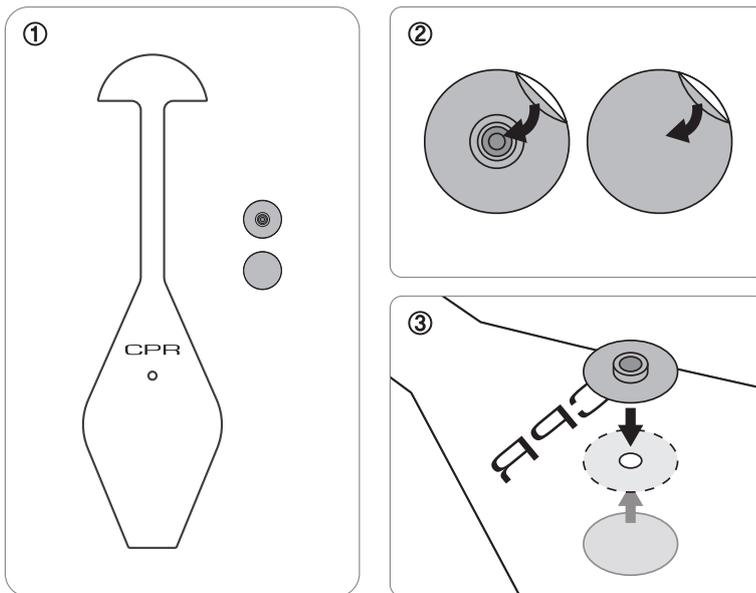

The sensor holders attached on the lung bag are reusable and can be attached to other lung bags multiple times, as long as the adhesiveness remains.

- ① Remove the lung bag from the manikin and prepare a new lung bag.
- ② Remove the sticker at the back of the breath module holder.
- ③ Attach sensor holders to the lung bag while matching the hole. Attach sensor holder A (silicon rubber) on the back of the lung bag, and sensor holder B (plastic) on the other side of the lung bag.
- ④ Install the completed lung bag.
*Refer to '3.2 Installing the lung bag' for how to install the lung bag.

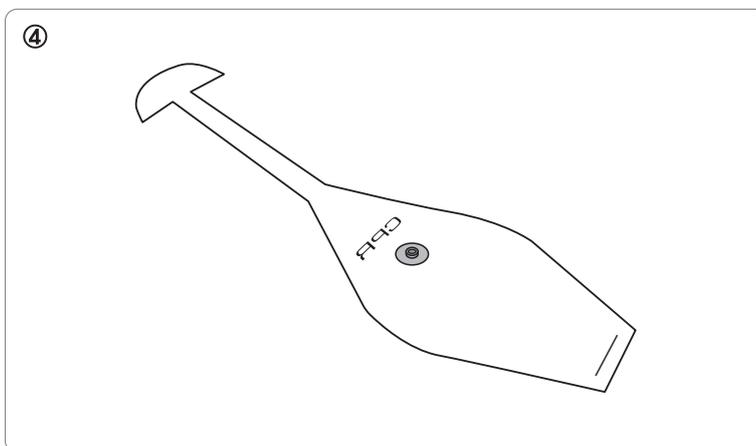


10. Troubleshooting

10.2. Frequently Asked Questions



Q. The app does not recognize the kit.

- A.** ① Please make sure LED is on.
② Push the power button to reset, or disconnect the kit from another app.

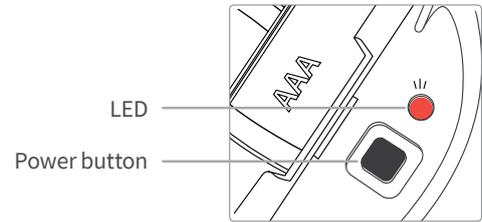

Q. The kit's LED is on but the app is not recognizing the kit.

- A.** If you're using 'HeartiSense' app not 'Add-on kit' app, the kit cannot be connected. Please search "Add-on kit" from the app store and download the correct app.

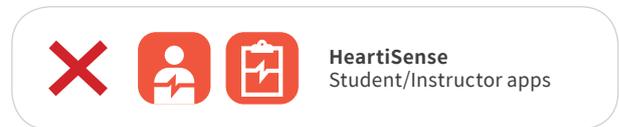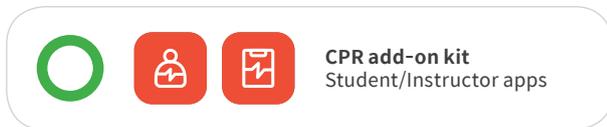

Q. Batteries are inserted but the kit's LED is not turning on.

- A.** ① Please make sure that batteries are properly inserted.
If the ends of the batteries are not touching the electrodes, the power wouldn't turn on.
② Please replace the old batteries with the new batteries.

Q. While using the app, the message "Low Battery" is shown.

- A.** Please replace the old batteries with the new batteries.



Q. When breath is delivered, manikin's chest rises (due to the air filled) but the app does not show any value.

- A.** Please check and make sure that the breath module is properly attached to the lung bag.

Q. Where can I check kit software(firmware) information?

- A.** For Student app, go to 'Settings' > 'Kit Information', then check 'Kit Software'.
For Instructor app, go to 'Link' tab, then choose the kit you wish to check the information for further details.
*Please refer to section 8.5.

Q. Where can I check app version?

- A.** Go to 'Settings' > 'App Version'.
*Please refer to section 8.6

10.2. Troubleshooting

Symptom

While trying to connect with the kit, the message "Connection Failed" is shown.



Or the icon on the left is shown.

Breath module is properly connected but the value shown is not correct.

During CPR session, within 5 minutes and 5m distance range, the connection with the kit continues to be lost.

Cause

The breath module is not good to use and needs to be replaced.

The breath module is not good to use and needs to be replaced.

The saved breath calibration value might be wrong so that the appropriate breath volume cannot be shown.

The mobile device you're using is not compatible with the kit.

The kit software is outdated.

The connection might be lost if there is an obstacle between the kit and the user's mobile device.

Troubleshooting

Separate the breath module from the kit and connect a new breath module to the kit.

*Refer to section 9.3.

Separate the breath module from the kit and connect a new breath module to the kit.

*Refer to section 9.3.

Open the 'Kit Information' screen, then press the 'Calibration' button to recalibrate the breath sensor.

Recommended technical specification for mobile devices:

- Models after 2017
- Devices with BLE version equal to or above 4.2
 - * Low-cost devices with BLE version equal to or above 4.2 might still have connection issues
- iOS: OS version equal to or above 11, iPhone 6S or models after 6S is recommended (Some outdated iPods might be exceptions)
- - Android: OS version equal to or above 6.0 Marshmallow (certain low-cost devices are exceptions)

Refer to the section '8.5. Checking the kit information ' and check 'Kit software'.

Update is required if the firmware version is below 1.1.1. Please contact customer service center.

Please make sure that there is no obstacle between the kit and the user's mobile device.

11. Warranty

1. Manufacturer offers a LIMITED WARRANTY against any defects in workmanship or materials under normal use for one (1) year from the date of purchase. Any component of the BasicBuddy®plus add-on kit which proves defective within the warranty period will be repaired, free of charge. The customer is responsible for shipping and handling fees to the place which manufacturer designates.
2. Customer must provide proof of the date of purchase, place of purchase and the purchase price in order to obtain service under this limited warranty. No agent, representative, dealer of Manufacturer has the authority to alter the obligations or limitations of this limited warranty.
3. CUSTOMER'S SOLE AND EXCLUSIVE REMEDY AGAINST MANUFACTURE SHALL BE FOR THE REPAIR OR REPLACEMENT OF DEFECTIVE GOODS AS PROVIDED HEREIN. Repair of any component of any BasicBuddy®plus add-on kit does not extend this limited warranty or begin a new limited warranty period.
4. Manufacturer reserves the right to refuse warranty service or replacement when product failure is due to abrasion, abnormal use, misuse, mishandling, misapplication, accident, neglect, improper installation, modification, use of unauthorized parts or attachments, adjustments or repair performed by anyone other than manufacturer or its authorized agent, or any causes other than defective workmanship or material. This limited warranty does not cover failure or damage resulting from unsuitable operating environments or storing environments or natural disasters or acts of God. MANUFACTURER SHALL NOT BE LIABLE FOR INCIDENTAL OR CONSEQUENTIAL DAMAGES ARISING OUT OF THE USE OF THE BasicBuddy®plus add-on kit OR THE BREACH OF THIS OR ANY OTHER EXPRESSED OR IMPLIED WARRANTY.

12. Contact



Homepage www.NascoHealthcare.com
Address 901 Janesville Ave.
Fort Atkinson, W153538

E-mail lifeform@enacso.com
Phone 1.800.431.4310